

Estd. 1966



Clinical Middle Ear Analyzer R 36 M (MODEL NO : DIAU 150)



DELIVERING TO THE WORLD

Clinical Middle Ear Analyzer R 36 M Manufactured by Desco Medical India




Decide with Confidence

Clinical Middle Ear Analyzer R 36 M

Estd. 1966



DELIVERING TO THE WORLD

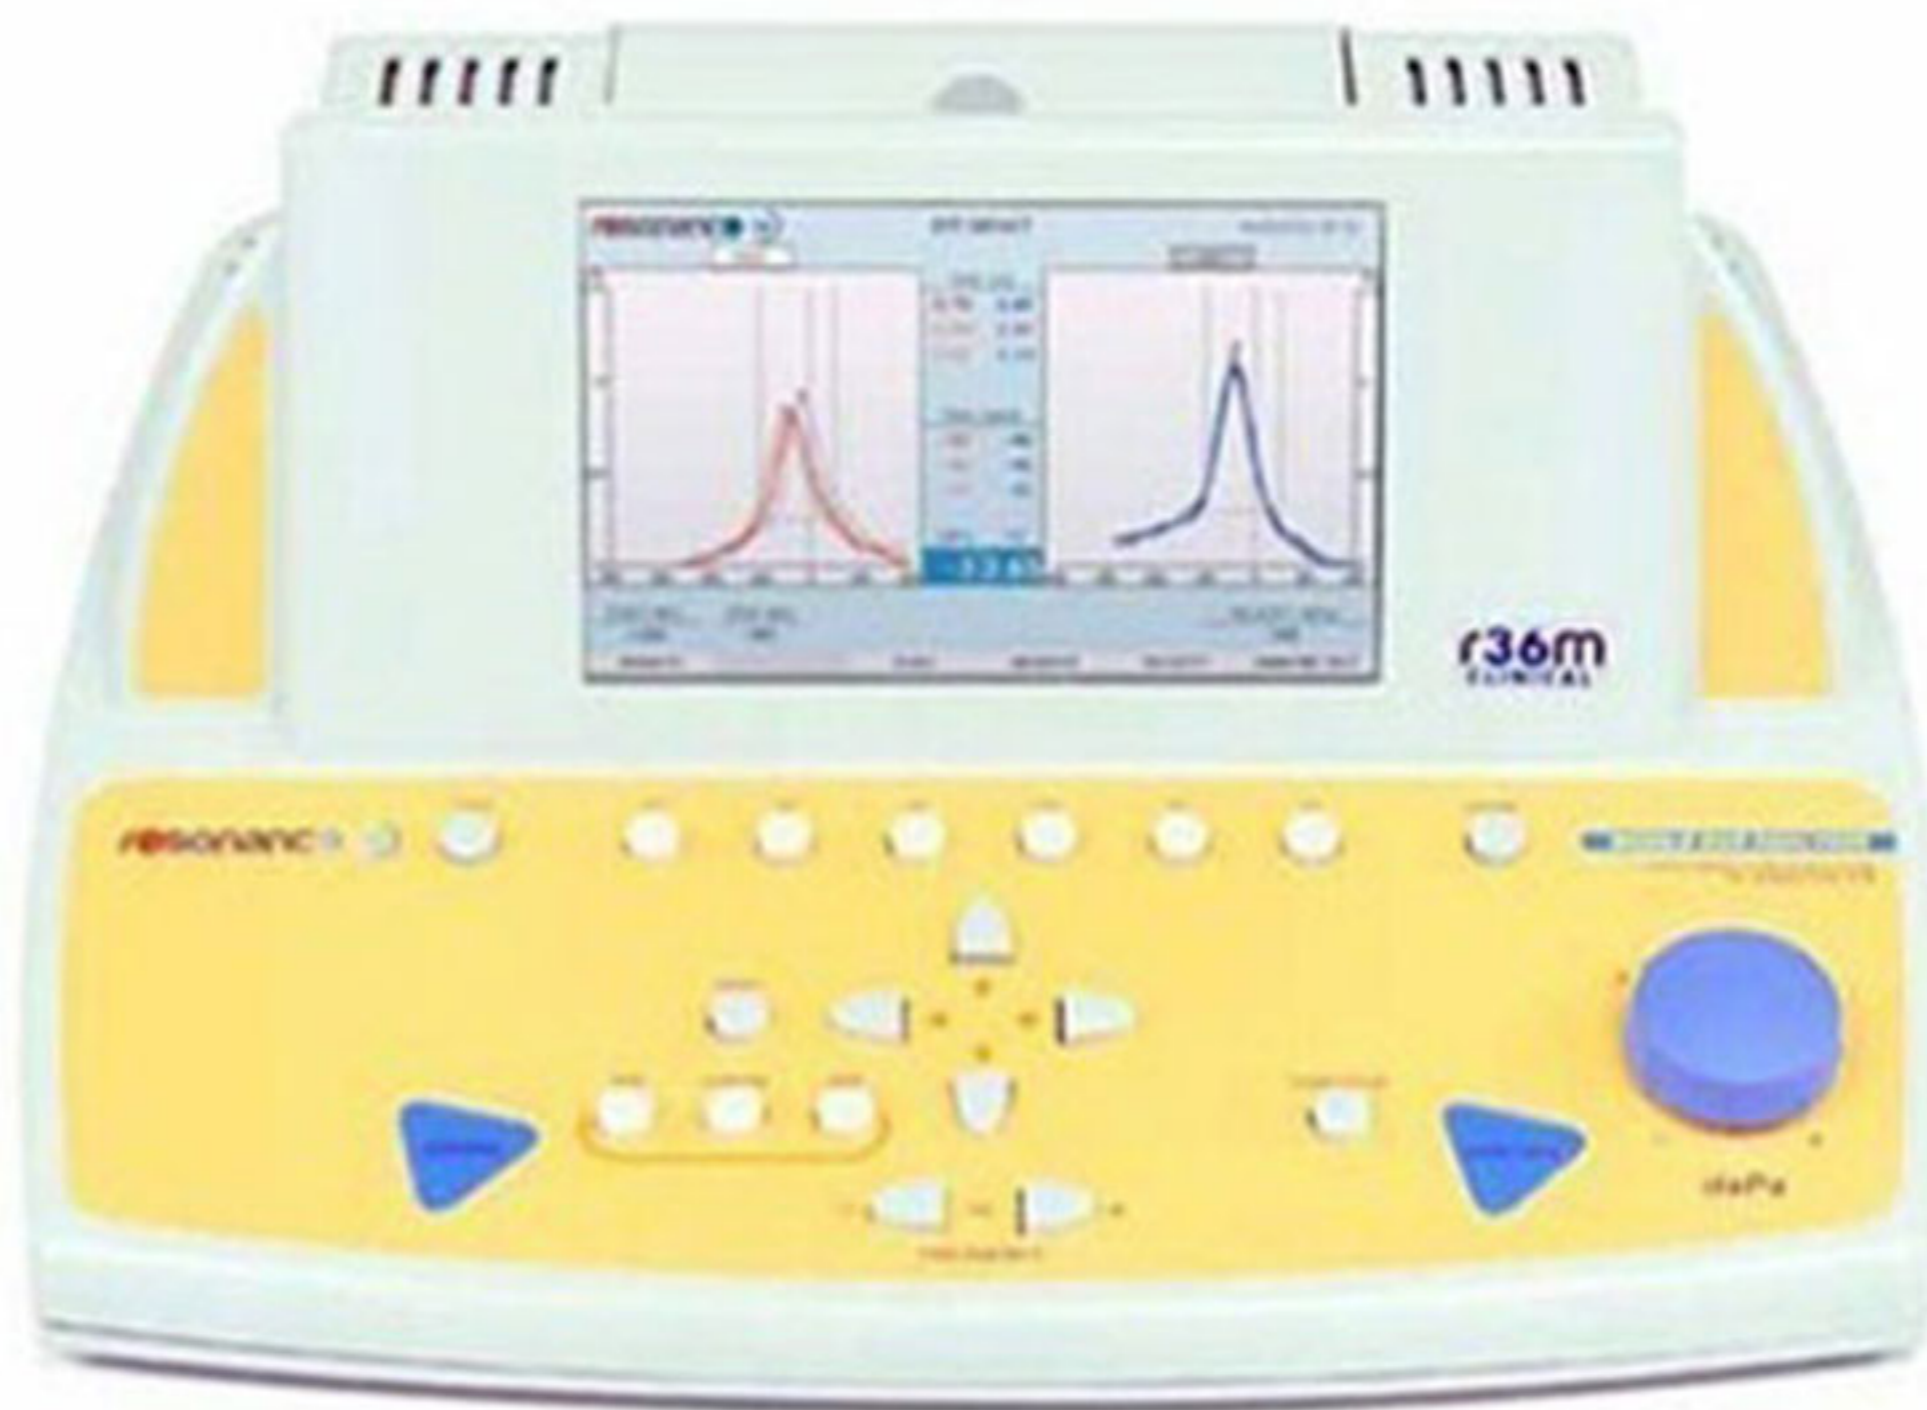

www.descomedicalindia.com

www.descoonline.in



Clinical Middle Ear Analyzer R 36 M (MODEL NO : DIAU 150)



Clinical Middle Ear Analyzer R 36 M Manufactured by Desco Medical India

Specifications :-

Clinical Middle Ear Analyzer is used for Tympanometry acoustic reflex measurement. Compact dimensions, excellent ergonomics and a luminous 7" TFT display: R36M has been engineered to respond to the needs of ENT and Audiology Specialists, operating both in clinic and at patient domicile. Design is user-friendly and allows both device and accessories to be safely carried around in a carrying case, available on demand. R36M offers several options for managing and archiving .pdf test-report files. Pdf test-report files can be initially stored in a USB-stick and then either archived into external units or printed thanks to the built-in thermal printer. Reports can be easily edited and customized with additional texts and logos. MDS Suite software allows patient data and tests results transfer to PC. R36M is built upon a 30-years experience and know-how gained in the audiological industry by Resonance®. This device offers a complete range of clinical Tympanometry tests. The R36M in -PT configuration includes Multifrequency Tympanometry. All configurations aim to simplify daily operations and maximize efficiency. Design of accessories maximizes patient comfort for the best and easiest handling of the device. Optional accessories increase flexibility and performance.

TEST TYPES • Tympanometry: Automatic Tympanometry, Acoustic, Reflex, Reflex Decay, Quick test: check, screening and Decay, Acoustic Reflex Latency Test (ARLT), Multifrequency Tympanometry*, ETF (Intact, Perforated and Patulous), Special tests (Growht-DLI and Non acoustic)

USER INTERFACE • Multilingual. **PRINTER** • Built-in fast thermal printer with paper width: 112 mm supplied as standard part. **REPORTS** • Printed on thermal printer, •.pdf report created directly from the device and stored on USB Pen drive with possibility to add patient data and tests comments via the USB Keyboard (optional), • Data transfer to PC using Resonance Management Data Suite. **"CHILDREN" FEATURE** • To help keep the child distracted while running screening, "Quick Check" a series of animated images appears on the color display. **COMMUNICATION PORT** • Nr.1 USB host type A • Nr.1 USB slave type B. **WINDOWS® COMPATIBLE SOFTWARE**, • Resonance MDS Management Data Suite. Tympanometry Specifications

PROBE TONE • 226 Hz for Admittance (Y) curve tympanometry, • 678, 800 and 1000 Hz for multifrequency tympanometry with added "B" and "G" curve *. **INTENSITY** • 226 Hz: 85dB SPL ± 2dB, • 678, 800 and 1000 Hz: 75dB SPL ± 2dB*

• Frequency Accuracy: ± 0,5%, • Harmonic distortion: Less then 1%. **ADMITTANCE MEASUREMENTS** • Compliance range at 226Hz: 0,05 up to 7ml. • Sensitivity scale: Autoscale to appropriate range; available scale at 226Hz: 1.5, 2, 5ml or 7ml

• 678, 800 and 1000 Hz: 0 to +25 mmho*, • Sensitivity scale HF: Autoscale to appropriate range, available scales at 678, 800 and 1000Hz: 5, 10, 15, 20, 25 mmho*. **AIR PRESSURE** • Control: Automatic and Manual, • Range: from +400 up to -600 daPa adjustable in 50 daPa steps, • Sweep rate: 50, 100, 200,300 daPa/sec and automatic, • Indicator: Measured value is displayed

• Safety limitations: -800 up to +600 daPa, • Pressure accuracy: ± 10 daPa or ± 10%

EUSTACHIAN TUBE FUNCTION • ETF test for use with both intact and perforated eardrums. **ACOUSTIC REFLEX TESTS**

• Reflex test method: Threshold , Automatic, Manual, • Stimulus duration: 0,5 , 1 or 2 sec., • User selectable protocols for all test methods, • Ipsi or Contralateral stimulation for all reflex test, • Automated peak search functions available for all test methods, • Manual Reflex: manual control of all stimuli, • Reflex Decay: Threshold , Automatic, Manual Stimulus duration: 10 or 20 sec., • ARLT: Threshold , Automatic, Manual Stimulus duration: 1 sec. fixed, • Non Acoustic: 10/20 sec.

• Reflex test method: Threshold , Automatic, Manual, • Stimulus duration: 0,5 , 1 or 2 sec., • User selectable protocols for all test methods, • Ipsi or Contralateral stimulation for all reflex test, • Automated peak search functions available for all test methods, • Manual Reflex: manual control of all stimuli, • Reflex Decay: Threshold , Automatic, Manual Stimulus duration: 10 or 20 sec., • ARLT: Threshold , Automatic, Manual Stimulus duration: 1 sec. fixed, • Non Acoustic: 10/20 sec.

FREQUENCIES AND INTENSITY RANGES • Ipsilateral: – Pure tone level range (dBHL) from 50 to 110 (all version)

– Noise level range (dBSPL) from 50 to 100 (all version), • Frequency: 500, 1000, 2000, 3000, 4000 Hz, BBN,HP or LP noise

• Accuracy: ±1%, • Harmonic distorsion (THD): less than 3%, • Contralateral: – Pure tone level range (dBHL) from 50 to 120 (all version), – Noise level range (dBSPL) from 50 to 115 (all version), • Frequency: 250, 500, 1000, 2000, 3000, 4000, 6000, 8000 Hz, BBN,HP or LP noise, • Accuracy: ±1%, • Calibration accuracy ±3 dB, • Level steps: 1, 2, 5 or 10 dB

• On/Off ratio: 70 dB minimum, * R36M-PT only

We are Manufacturer, Exporters and Suppliers of Clinical Middle Ear Analyzer at wholesale competitive prices from India.